

Capnograph

Model: Capno Cube

USER MANUAL



Shenzhen Creative Industry Co., Ltd.
V1.1 19/11/2019

This Manual is written and compiled in accordance with the IEC 60601-1 (Medical electrical equipment Part1: General requirements for safety) and the General Principles of GB/T9969-2008 User Manual for Industrial Products issued by the State Technological Supervision Bureau of China. It complies with both international and enterprise standards and is also approved by State Technological Supervision Bureau. The Manual is written for the current Capno Cube Capnograph. The Manual describes, in accordance with the Capnograph's features and requirements, main structure, functions, specifications, correct methods for transportation, installation, usage, operation, repair, maintenance and storage, etc. as well as the safety procedures to protect both the user and equipment. Refer to the respective chapters for details. The Manual is published in English and Creative have the ultimate right to revise or modify the Manual. All rights reserved.

Marks in the Manual:

Warning: must be followed to avoid endangering the operator and/or the patient.

Attention: must be followed to avoid causing damage to the monitor.

Note: some important information and tips about operations and application.

Caution:

In some countries Federal law restricts this device to sale by or on the order of a physician.

Notice

Welcome to user manual for the Capno Cube Capnograph. This manual includes the materials and copyright is reserved. It is not allowed to copy, reduplicate or translate into other languages without our written permission. Please to read this manual carefully before use and then operate the Capno Cube by following the instructions of this manual. It is not allowed to open the monitor's cover without our permission. If any software revisions are made, it must be notified by the monitor's cover. Software revisions must be altered by the built-in user interface. Some changes to the product due to the technology updates or improvements or due to the special demands of the user which do not influence the monitor's key functions will not be informed further. Furthermore please pay attention to the difference between the parts or components and this manual. Please contact Creative for technical documents or electric circuit diagram or relevant batch and lists of parts or components etc.

**Shenzhen Creative Industry Co., Ltd. Add: Floor 5,
BLD 9, Baiwangxin High-Tech Industrial Park,
Songbai Road, Xili Street, Nanshan District, 518110,
Shenzhen, China**

Tel: +86-755-2643 3514 Website: www.creative-sz.com

CONTENTS

Chapter 1 Preface	1
1.1 Brief	1
1.2 Warranty and Maintenance	1
1.3 Safety Requirements	2
Chapter 2 Technical specifications and characteristics	8
Chapter 3 Introduction of Monitor	14
Chapter 4 Patient connection	17
4.1 CO ₂ measurement	17
4.2 Respiration rate measurement	18
4.3 The sensor's zero	19
4.4 Notice	20
Chapter 5 Screen display and Operation	21
5.1 Screen main display menu	21
5.2 The Main Menu	26
5.3 CO ₂ SET Menu	27
5.4 TIME SET Menu	29
5.5 NEW PATIENT Menu	31
Chapter 6 Charging, Maintenance, Cleaning	33
6.1 Charge	33
6.2 Maintenance	34
6.3 Cleaning	34
Chapter 7 Trouble Shooting Analysis	36
Appendix 1. Explanations of Terms in this Manual	38
Appendix 2. ENGINEER MENU: Changing compensation of balance gas	39
Appendix3. Guidance and manufacturer's declaration – Electromagnetic compatibility	41

Chapter 1 Preface

1.1 Brief

The purpose of this manual is to provide the User with a brief understanding of the characteristics, functions and operation of the monitor thereby preventing incorrect operation and user error. This device can monitor two physiological parameters for the patient at the same time: End tidal CO₂ concentration (EtCO₂),

1.2 Warranty and Maintenance

Respiration Rate (RR).

Warranty 1 Year Warranty on Hardware and Battery

This Monitor has a warranty of 12 Months from the date of purchase.

All the Accessories have a warranty of 6 months or “out of box” for Disposable Items.

The following will invalidate the warranty:

- if the monitor is damaged due to misuse or incorrect operation (i.e. without following the User manual instruction),
- the monitor is damaged due to incorrect connection with another instrument.
- the monitor is accidentally damaged or dropped
- if the user modifies or changes the monitor without written authority of the company.

- the serial number is deliberately damaged, torn off or unreadable.

Maintenance

If the monitor is non-functional outside of the warranty period, the manufacturer or distributor will offer an estimate for repair. The maintenance/repair/calibration place depends on actual conditions.

Re-packing for Repair or Calibration

It is recommended to use the original packing boxes and packing materials when returning for repair or maintenance.

1.3 Safety Requirements

For the purposes of safety, please read the following and abide by these instructions of medical instrumental products.

Warning: Indicating the possible injury on patient or operator.

General

- **Warning:** To ensure accurate performance and prevent device failure, do preventive maintenance inspection (including performance and safety check) each 6 to 12 months to verify that the monitor operates & functions correctly & is in good condition to ensure patient and medical personnel safety.
- **Warning:** Check the safety and performance of this monitor every time before using it to ensure it works normally and safely.

User Manual of Mainstream Capnograph

- **Warning:** This monitor should be used for only one patient at the same time.
- **Warning:** This capnograph is intended only as an adjunct in patient assessment, not a treatment device, nor an equipment used in home.
- **Warning:** If uncertain about the accuracy of any measurement, first check the patient's vital signs by any alternate means, and then make sure the monitor is fully functional.
- **Warning:** This device should not be used as an apnea monitor.
- **Warning:** To ensure patient safety, do not place the monitor in any position that may cause it to fall on the patient.
- **Warning:** DO NOT lift the monitor by the cables and hoses of the applied parts, as they could disconnect from the monitor, causing the monitor to fall on the patient.
- **Warning:** If the monitor falls or impacts accidentally, please do not operate it until its safety and performance have been carefully tested and positive testing results obtained.
- **Warning:** DO NOT position the sensor cables or tubing in any manner that may cause entanglement or strangulation.
- **Warning:** To ensure accurate performance and prevent device failure, do not expose the monitor to extreme moisture, such as rain.
- **Warning:** The use of accessories, sensors power adapter and cable other than those specified with the equipment may result

User Manual of Mainstream Capnograph

in increased emission and/or decreased immunity of the equipment or other systems.

- **Warning:** Airway Adapter is for single use only. Reuse of the single use Adapter can cause cross infection.
- **Warning:** CO₂, respiratory rate readings and signals can be affected by sensor application errors, certain ambient environmental conditions, and certain patient conditions.
- **Warning:** The monitor is a prescriptive device and is to be operated by qualified healthcare personnel only.
- **Warning:** When disposing of the device or accessories& its packing, local laws and regulations should be followed.
- **Warning:** This monitor provides End tidal CO₂ (EtCO₂) concentration, Respiration Rate. This data only provides assistance for diagnosis and actual diagnosis shall be made by suitably qualified clinical staff using all the clinical information and symptoms.
- **Warning:** Biocompatibility tests have been performed on all the applied parts, some exceptional allergic patients may still have anaphylaxis. Do not apply to those who have anaphylaxis.
- **Warning:** do not modify this equipment without authorization from the manufacturer.
- **Warning:** The alarm setting values could be restored automatically within 30 seconds of loss of power.
- **Warning:** The design life of this capnograph is 5 years. The

capnograph shall be collected and recycled in accordance with local law after 5 years. Please contact with local agency or manufacturer for any questions.

MRI scanning

- **Warning: MR-unsafe! DO NOT allow this device to enter an MRI environment**
- There are some electromagnetic or inductance circuits designed into the device. Use in an MRI environment could cause burns or adversely affect the MRI image or the device's accuracy.

Warnings:

DO NOT expose the device to a magnetic resonance (MR) environment.

- The device may present a risk of projectile
- Injury due to the presence of ferro—magnetic materials that can be attracted by the MR
- Magnet core.
- Thermal injury and burns may occur due to the metal components of the device that can heat up during MR scanning.
- The device may generate artifacts in the MR image.
- The device may not function properly due to the strong magnetic and radiofrequency fields generated by the MR scanner.

Alarms

- **Warning:** Do not silence the audible alarm if patient safety may be compromised.
- **Warning:** Always respond immediately to a system alarm since the patient may not be monitored during certain alarm conditions.
- **Warning:** Before each use, verify that the alarm limits are appropriate for the patient being monitored.
- **Warning:** Check the audible alarm silence duration before temporarily silencing audible alarms.

Fire Hazard

- **Warning:** The monitor is not suitable for use in the presence of flammable anesthetic mixture with air, oxygen or nitrous oxide.

Electrical

- **Warning:** To protect against electric shock hazard, the monitor's cover is to be removed only by qualified service personnel. There are no user-serviceable parts inside.
- **Warning:** To ensure patient electrical isolation, connect only to other equipment with circuits that are electrically isolated.
- **Warning:** Refer service to qualified service personnel.
- **Warning:** Do not open the sensor cabinet at will, as electric

shock hazard may occur.

- **Warning:** Measure the device's leakage current whenever an external device is connected to the serial port. Leakage current must not exceed 100 microamperes.
- **Warning:** Electrical installation of the room or the building in which the monitor is to be used must comply with regulations specified by the country in which the equipment is to be used.

Electro-Magnetic Interference

- **Warning** Operating high frequency electrosurgical equipment in the vicinity of the monitor can produce interference in the monitor and cause incorrect measurements.
- **Warning:** Do not use the monitor with nuclear spin tomography (MRT, NMR, NMT) as the function of the monitor may be disturbed.

Indication for Use

The Capnograph is designed for monitoring the vital physiological signs of the patient. It is use for non-invasive continuous monitoring of EtCO₂ and Respiration Rate.

The Capnograph is indicated for in patients from newborn (neonate) to adult in a hospital environment. It is intended to be

used only under regular supervision of clinical personnel

Chapter 2 Technical specifications and characteristics

EtCO₂ Method: Creative proprietary non-dispersive InfraRed Spectroscopy

Range: 0 – 150mmHg or 0 – 20kPa or 0 – 20% (v/v)

Accuracy: ± 2 mmHg for EtCO₂ range 0 - 40mmHg,
 ± 5 % for EtCO₂ range from 41 - 70mmHg
 ± 8 % for EtCO₂ range from 71 - 100mmHg
Over 100mmHg ± 10 %

Note1: The accuracy of CO₂ concentration measurement is influenced by any interfering gas and/or vapour, for example N₂O gas can raise the CO₂ reading (2-10%), and Helium and O₂ can reduce the CO₂ reading (1-10%), so compensation should be set in the balance gas MENU to meet the accuracy requirements if such gases or vapours are present.

Note2: The accuracy of CO₂ concentration measurement is also influenced by Respiration rate. The corresponding relationship is follows:

Table1 EtCO₂/ Respiration Rate Accuracy

EtCO ₂ (mmHg)	Respiration Rate	Accuracy
0 - 40	0-79	±2mmHg
	>80	±12%
41 - 70	0-79	±5%
	>80	±12%
71 - 100	0-79	±8%
	>80	±12%

User Manual of Mainstream Capnograph

>100	0-79	$\pm 10\%$
	>80	$\pm 12\%$

Test method:

As shown in table 1, test the accuracy of different concentrations of gas at different respiratory rates. Set up the gas flow rate of 1 L/min, the sampling rate is 100ml/min. And then record the data.

When device in real time measures CO₂ in the breathing loop, and during CO₂ in the gas loop is evacuated and its

measured is decreased and reaches zero, when exhaling, CO₂ enters the breathing loop and its concentration rises rapidly and is kept at a certain platform, at the end of expiration (end tidal) it reaches maximum.

In this repeated way, a real-time and high or low waveform is formed by the virtue of this waveform, the device calculates the respiration rate and also by measuring respiration cycle, the device meantime calculates the respiration rate.

Update/Averaging Time: Option of every breath

Warm Up Time: <15 seconds

Rise times (t₁₀₋₉₀ %): About 70ms

Memory: 24 hours on Screen Trend & Numeric

Inspiratory CO₂

Range: 3~50mmHg

Respiration Rate

User Manual of Mainstream Capnograph

Range:	0 - 150 rpm
Accuracy:	$\pm 1\%$ of reading / ± 1 rpm whichever is greater
Memory:	24 hours on Screen Trend & Numeric
Sensor:	Adapter for intubated Patients

Alarm limits

High alarm limits EtCO₂: 22-99mmHg (2.93-13.2 kPa)

Low alarm limits EtCO₂: 20-99mmHg (1.33-8.0 kPa)

The high alarm limits of respiration rate: 5-60 breaths/min

The low alarm limits of respiration rate: 4-40 breaths/min

Power

AC Input: 100V - 240V, 50Hz/60 Hz to 5VDC Adapter with 5V mini USB adapter Cable.

Battery

Type: Built-in rechargeable lithium battery pack (3.7V, 1400mAh)

Charging Time: 4 hours from flat

Operating Time: 6 hours on full charge

Operating

~~Conditions~~ Temperature: 5 to 40°C

Humidity: 30%~75%

Atmospheric pressure: 86-106 kPa

Storage Conditions

Temperature: -30 to +70oC

Humidity: <93% (non-condensing) =< 29.45 hPa

Atmospheric pressure: 50 - 120 kPa

Dimensions of Monitor

Size: 38 x 42 x 44mm (W x H x D)

Weight: 80g (including lithium battery and adult airway adaptor)

Warranty & Maintenance/ Calibration

One year warranty on Main Unit and Lithium Ion Rechargeable Battery

IP rating

IP33

CE & Product classification

As per IEC 60601- 1 / CSA601.1 / UL2601-1

Type of Protection

Class II

Degree of Protection: Type BF-Applied Part

Mode of Operation: Continuous

Airway Adapter

Dead Space: 5ml (Adult/Paediatric)

1ml (Neonate)

93/42/EEC Medical Device Directive Compliant

EC-Representative:

Shanghai International Holding Corp. Gmbh (Europe)

Eiffestraße 80, 20537 Hamburg Germany

CE 0123


Chapter 3 Introduction of Monitor



Figure 1

(1)Screen: Displays waves, menu, alarm and all measuring parameters.

(2)S-button: Press this button to move the cursor when menu is activated.

(3) : When menu is activated, to press this button as confirmation button or increase (+) button.

(4) : multifunction button

- a) When menu is activated, to press this button to decrease data selected.
- b) In the main display screen, to press this button to silence alarm for two minutes.
- c) In the main display screen, to press this button over 2 seconds, the display screen will change to big font display mode as the figure showing:



Figure 2

(5):  Multifunction button

- a) Power switch, to press this button for two seconds to turn on or turn off power.
- b) Press this button with a short fast press to enter or quit the menu.
- (6) Light indicator: Flickering green light indicates power adaptor is connected and green light indicates the device begins to work.

- (7) Battery compartment location
- (8) DC5V Mini USB Charging interface. Note: this interface must only be connected to a device which meets safety standards.
- (9) Hanging Point for Lanyard if required.
- (10) Airway adaptor

Note: The direction sensor is installed in the device so the screen display direction will be automatically adjusted according to the vertical direction of the device. Of course, the screen direction can also be set manually: First, enter the ENGINEER MENU and set screen rotate to manual. (see Appendix 2 for details.) Then, in the main screen, to press button S over 2 seconds, the display screen will counterclockwise rotate 90°.

Chapter 4 Patient connection

4.1 CO₂ measurement

Usage of the monitor

The device is a mainstream CO₂ sensor and maybe used immediately – just ‘zero’ the reading as in 4.3 with each new adapter tube.

Theory introduction

The principle is based on the fact that CO₂ molecules absorb

infrared light energy of specific wavelengths, with the amount of

energy absorbed being directly related to the CO₂ concentration. When an IR light beam is passed through a gas sample containing

CO₂, the electronic signal from an infrared sensor (which measures

the remaining light energy), can be obtained. This signal is then

compared to the energy of the IR source, and calibrated to accurately reflect CO₂ concentration in the sample. To calibrate, the

infrared sensor's response to a known concentration of CO₂ is

17

stored in the monitor's memory.

In addition, the circuit module has atmospheric absolute

User Manual of Mainstream Capnograph

Then the monitor (CO₂ module) determines CO₂ concentration in the breathing gases by measuring the amount of light absorbed by these gases. EtCO₂ is display as a numerical value in millimeters of mercury (mmHg), percent (%), or kilopascals (kPa). In addition, a CO₂ waveform (capnogram) may be displayed which is a valuable clinical tool that can be used to assess patient airway integrity and proper endotracheal tube placement. Respiration rate is calculated by measuring the time interval between detected breaths.

Connection and Installation

- 1) Install the airway adaptor on the monitor
- 2) Install the monitor into the patient's gas loop.

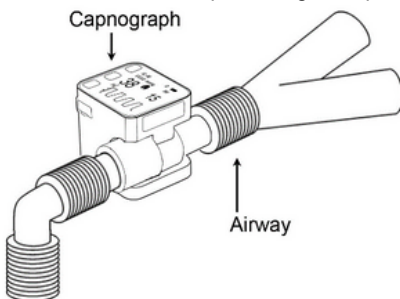


Figure 3

4.2 Respiration rate measurement

The calculation of respiration rate derives from monitoring the peak

to peak time from the CO₂ waveform.

4.3 The sensor's Zero for each new Adapter fitted

1) Zeroing the calibration The anti-fogging window of the airway adaptor has a certain

attenuation to infrared signal but due to individual diversity, its

attenuation is different. So the sensor needs to be zeroed when

changing new adapter. In addition, the sensor and infrared source

may have a small amount of natural drift with time. In this case the

sensor may need to be zeroed after long usage, if the data is not

correct.

Attention: Zeroing needs to be done carefully to prevent a false zero

calibration causing a deviation of measurement data.

ZERO! If this item is high-luminance colour that means the sensor's data is stable and it can be zeroed. Then press **←/→** button, send the Zero command and **ZEROING** will be shown. Connect the Adaptor with the Capno Cube and allow to warm up. Wait for 15-20 seconds till 'ZEROING' disappears. for 5-10 minutes.

Place the device into a free air space without CO₂ and do not breathe near it. Then, enter CO₂ setting submenu, move cursor to'

4.4 Notice

Caution:

Under the conditions of electromagnetic influence, for example: electrosurgical devices, MRI, CT etc. may negatively impact the devices performance. Attention: other important information.

The CO₂ readings may be inaccurate if the monitor does not warm

up sufficiently

ONLY Use the airway adaptor provided by the manufacturer,

otherwise measurement data might be not correct.

Measurement data might not be correct if used in fast temperature

change environment. Therefore, if a fast temperature change

happens beyond a certain range, 'TEMP IMBALANCE' will be

shown on the screen. If this occurs only use under more stable

temperature conditions.

When the device is used with anesthesia gas, the measurement

data will be an influenced unless it is calibrated for anesthesia

gases, please refer to Appendix 2.






Warning:

Chapter 5 Screen display and Operation

5.1 Screen main display menu



Figure 4

1. The first line of data shows time (hour, minute)/patient ID, the memory area full indicator (), silence () or non-silence , Bluetooth symbol () and battery indicator .

Attention:


a) When the memory full indicator is displayed, further patient data cannot be stored. If you want to save the new data effectively, you need to enter the NEW PATIENT menu to delete the data in the storage area, or to change patient ID. You can also set up trend RENEW into AUTO mode, please see the details in 5.5

NEW PATIENT b) The symbol () appears if the bluetooth module is enabled. If

this symbol is green, it indicates that no bluetooth equipment is

connected, if this symbol becomes white, it indicates that some

bluetooth equipment is connected.

2. The other part of the screen shows results data and (during exhaling,  becomes blue colour), CO2 respiratory wave.

5. CO2 concentration status, peritowhen taking away a patient, 'NO ADAPTER' will be shown on the screen, when the probe needs

zero calibration, 'ZERO REQ' will be shown on the screen to indicate that probe might need zero calibration.

Alarm setting:

The alarm settings of the system are LATCHING and will not change after shutting down the power of capnograph.

Alarming level:

There are two types of alarming: physiological alarm and technical alarm. Physiological alarm refers to the alarm causing by physiological change of patient, patient's life may in danger.

Technical alarm refers to system fault which cause capnograph working improperly or providing unreliable readings. This capnograph adopt only medium priority alarm.

Medium priority alarm means serious warning.

Warning: Medical personnel should set alarm limit based on clinical experience. DO NOT set values over maximum limit of alarm.

Warning: Same or similar device with different setting of alarm may cause potential danger in isolated area like ICU or operating room.

Please refer to the content of menu setting of CO₂.

It is critical to set alarm of physiological parameter which gives alarm clinical significance.

Alarm delay:

The sum of maximum delay of alarming state and signal generation is less than 10 seconds.

Alarm indication:

- 1) If the EtCO₂'s value exceeds the limit of high or low alarm level, the word 'EtCO₂' will flash and alert with the audible high priority alarm. This high priority alarm will also sound for respiration rate.
- 2) If the battery level is almost fully depleted the battery indicates completely empty, the monitor will alarm continuously and will shut down automatically.
- 3) When the no CO₂ detected alarm is turned on and no CO₂ detected occurs the monitor will give an audio/visual alarm. The screen will flash the message 'no CO₂ detected' (meaning no EtCO₂ has been detected for a certain time period) and 'Beep' sound will also be heard.

User Manual of Mainstream Capnograph

4) Symbol of parameter will turn yellow and blink if any over ranging parameter triggers alarm.

Alarm sound:

Alarm sounds as following protocol. Time interval cannot be changed.

Level of alarm	Sound	Sound pressure
Medium priority alarm	"Beep-Beep-Beep", triggered each 8 seconds	45~70dB

Alarm light:

Alarm light looks like following description.

Level of alarm	Light
Intermediate alarm	Parameter indicator turn yellow, blinking with frequency of 0.5Hz

Alarm silence:

In the main display screen (menu is not open), press the button



to silence the alarm for two minutes and the Alarm icon

becomes . Two minutes later, the Alarm silence will automatically

clear and the alarm will activate normally again if there is an alarm condition.

If you wish to cancel the alarm silence during the two minute period

then press the  button. When the two minute

Alarm Silence alarm is on, both physical alarm and technical alarm will be silent.

5) Any of the parameter alarms for over limits and no CO₂ detected alarm, will lead to the flashing of the red alarm indicator on the panel.

Alarm counter plan:

WARNING Always check status of patient if an alarm is triggered.

Check the alarm information displayed on the screen, correctly identify the alarm, and reasonably handle the alarm according to the cause of the alarm.

- ☒ Check patient's status.
- ☒ Identify type or parameter of alarming.
- ☒ Find the reason.
- ☒ Turn off alarming if necessary.
- ☒ Check alarm after removing alarming condition.

5.2 The Main Menu







Figure 5

In the main display screen, to press the button  to enter the setup menu, see the picture above.

In this menu, to press button S to move the cursor to choose item.

In this menu, to press button  to enter the next submenu, to press  again to go back to the main display screen.

This menu includes the following options:

The setting menu for CO2: CO2_SETUP

The time menu: TIME_SETUP

The new patient menu: NEW PATIENT.

WARNING: All Menu Settings are LATCHING and remain when



the Monitor is powered off. Ensure that all necessary settings are reviewed and are suitable for the patient BEFORE use.


5.3 CO2 SET Menu

CO2 SET		
EtCO2	ALAR H	50.0
	ALAR L	19.0
RESP	ALAR H	30
	ALAR L	08
APNEA TIME		30 S
CO2 UNIT		mmHg
ZERO		
WAVE SCALE		54mmHg
LOAD DEFAULTS		
EXIT		

Figure 6

In this menu, to press button S to move the cursor to choose item, to

press button  or button  to change data highlighted by the cursor.

If there are some actions not for changing data but just for direct operations such as LOAD_DEFAULTS or EXIT, then to press button +/  to execute.

In this menu, to press  button, then to exit this menu return back to the main display screen.

This menu includes the following setups:

- 1).The high alarm limits of EtCO₂: EtCO₂ ALARM_H: 22-99mmHg, off
- 2).The low alarm limits of EtCO₂: EtCO₂ ALARM_L: off, 0-99mmHg
- 3).The high alarm limits of respiration rate: RESP ALARM_H:5-60t/m, off
- 4).The low alarm limits of respiration rate: RESP ALARM_L: off, 4-40t/m
- 5). The setup of no CO₂ detected time: no CO₂detected TIME: 15s-44s, off
- 6).The unit of CO₂:CO₂ UNIT: %, mmHg or kPA
- 7).Sensor zero Calibration 8).CO₂ Wave scale: WAVE SCALE: 54mmHG or 76mmHG
- 9).Default reload: LOAD-DEFAULTS
- 10). Exit: EXIT

Attention:

- a) When respiration wave comes and EtCO₂ is not zero value, the

~~zero~~ Disturbance when ZERO will be dark colour and zero calibration

operation cannot be run;

Only when the sensor is in clean air without respiration wave and

User Manual of Mainstream Capnograph

calibrated, but must be sure without breathing near the sensor during zero calibration

b) The wave scale means the maximum value of waveform amplitude display but it does not mean data on full-scale. Data on full-scale still means 99mmHg.

Default values as follow:

EtCO₂ alarm high limit: 50 mmHg

EtCO₂ alarm low limit: 19 mmHg

RESP alarm high limit: 30 rpm

RESP alarm low limit: 08 rpm

No CO₂ detected time: 30S

CO₂ unit: %



WAVE SCALE: 54mmHg

5.4TIME SET Menu

TIME SET	
YEAR	13
MONTH	01
DATE	10
HOUR	21
MINUTE	18
SAVE	
EXIT	


Figure 7

In this menu to press button S to move the cursor to choose item,

to press button  or button  to change data highlighted by the cursor.

Attention: Any time adjustment will delete any stored trend data, so please take care before making this adjustment.

The procedure is as follows:

- 1) Change time.
- 2) Move the cursor to SAVE then press  button to enter the following menu FIGURE 8;
- 3) YES is already selected (highlighted in white) and if you wish to confirm this change press Enter if you do not wish to confirm the change move the cursor and highlight NO and press Enter.
- 4) Only by confirming can the time adjustments be made.





Figure 8

In the menu (Figure 7,8), to press  button to exit this menu without saving or changing data.

5.5NEW PATIENT Menu







Figure 9

In this menu to press button S to move the cursor to choose item,

to press button +/-  or button  to change data highlighted by the cursor.

In this menu, press  button, to exit this menu and enter the main display screen.

This menu includes the following setups:

- 1).**CLEAR MEMORY**: to delete all the historical data so as to store new data
- 2).**MEM**: to change store mode between manual data deletion

(STOP WHEN FULL) and automatic overwriting of the oldest data (AUTO LOOP).

3).**ID**: patient's ID, 00-99 optional

4).**SAVE**: to store the changed data (this needs to be confirmed by the new menu due to possibly substitution to the original data of the same ID of patient)

5).**EXIT**: to quit the current menu but not to store the changed setup

Chapter 6 Charging, Maintenance, Cleaning

6.1 Charge

Connect the AC/DC power adapter via the Mini USB port turn on the unit. The unit will charge the battery with power at the same time as operating. The battery charge will end after battery is full. The battery of this unit is a long life rechargeable lithium battery. When the unit is operated on battery only the battery indicator shows the battery's charge level on the screen. When the battery and the external 5VDC power must be connected as soon as possible. After DC power is connected, the monitor will recharge the battery, and will stop charging after the battery has fully recharged. Operation time for a fully charged unit is >6 Hours. Charge time is approx. 4 Hours.

Battery replacement method:

Note that the operation must be done with the DC Charger disconnected ensuring that the operator's safety is not compromised.

Press down and slide off to remove the battery cover, then carefully disconnect and remove the battery. Reverse this procedure to replace the new battery and re-fit the battery cover.

NOTE: Any battery that is removed and no longer required must

be properly disposed of by following national and local regulations.

6.2 Maintenance

If the monitor appears abnormal (e.g. system halted), to force the Monitor to shut down the press the Off switch for more than 5 seconds. Adaptor: If it is polluted or shown ADPTER ERR, you will need to replace the adapter and perform a zero calibration. **Attention:** Check adaptor before usage every time and check infrared window surface is in a clean condition.

6.3 Cleaning

Warning Before cleaning the monitor, device power must be turned off and removed from any charging source.

1) Cleaning the Monitor

It is recommended that the Monitor is always used in the supplied Rubber Bumper Case which offers considerable extra protection from contamination, liquid ingress and damage.

Do not to sterilize the Monitor by high pressure, autoclave or washer

Do not to dip or expose the Monitor to liquid

Do not to use the Monitor if there is any sign of damage

Use only PH Neutral Cleaning products.

User Manual of Mainstream Capnograph

This product is not suitable for mechanical re-processing or sterilization.

Monitor Cleaning Instructions:

Only the Rubber Bumper / Carry Case and if necessary the Monitor surfaces may be cleaned and/or disinfected. Use Moist (not dripping) wipes with 70% solution of isopropyl alcohol, or very dilute Chlor-clean (1000ppm) or Chlorohexidine (1000ppm) or mild detergent, then allow to air dry naturally.

2) Cleaning and sterilizing of the sensor's window and the airway adapter

Do not make high pressure sterilization sensor.

Do not steep sensor in the liquid.

a) Main device sensor window:

Use cotton swab or cloth strip wetted by clean water to graze and remove dirt and naturally air dried. Be sure it is dry before usage.

b) Cleaning and sterilizing of Single Use Adaptor:



Attention: This is a Single Use Adaptor and should not be re-processed. Use a new Adapter for each patient.

Chapter 7 Trouble Shooting Analysis

Simple analysis of problems

No.	Phenomena	Causes	Solution
1	The values of CO ₂ is lower	1. Leakage of gas loop 2. Need zeroing 3. The window of adaptor has fogging (low temperature) 4. Long used parts drift.	1. Check and replace gas loop and adaptor. 2. Sensor zeros. 3. Wait for the temperature rising 4. Recalibrate by the standard gas.
2	CO ₂ concentration is zero: .Show 'NO ADAPTER ' or 'SENSOR ERR' or 'IR LAMP BAD' on the screen.	1. Adaptor not fitted 2. Sensor data wrong 3. Light source wrong.	1. Check adaptor is plugged in 2. Check adaptor if plugged into correct position or infrared window has blot. 3. Contact manufacturer
3	Screen indicating CAL-ERR	The last calibration is failed.	Recalibrate by the standard gas.

User Manual of Mainstream Capnograph

4	The CO ₂ wave is not normal. Screen indicating TEMP-HIGH Or TEMP-LOW Or TEMP-IMBALANCE Flashing red	1. Temperature too high. 2. Temperature too low. 3. Temperature sharp change	To provide normal environmental temperature.
5	 closed down automatically.	1. Battery lack of power.	1. To connect AC /DC power adapter.
6	Still flashing red colour  after the power is supplied and AC indicator no light.	AC/DC power adapter working abnormally.	1. To check the AC/DC adapter and cable.

Attention: Please to contact the client' service centre if some problems occurred repeatedly.

Appendix 1. Explanations of Terms in this Manual


MENU	Menu
EtCO₂	The CO ₂ concentration of expiration end
RR	Respiration rate
mmHg	Millimeters Mercury
kPa	Kilopascal
ALAR H	Alarm high limit
ALARL	Alarm low limit
No CO₂ detected	No CO ₂ detected or breathing stopped for a set period of time
CAL	Offset Calibration
N₂O	Nitrous oxide
HELIUM	Helium gas
O₂CONCENT	O ₂ concentration compensation
ANAESTHETI C	Anesthetic gas
ZERO GAS	Base point or Zero point
BTPS	Temperature and deep lung air pressure compensation
CALIBRATE	Calibration
CANCEL:	Cancellation

Appendix 2ENGINEER MENU: Changing compensation of
balance gas

Attention:



Only trained personnel may carry out the following the procedure.
Contact your Supplier for training and advice.


Enter the engineer menu as follows:

When the device is powered on, entering version display window,
simultaneously to press both button S and button  to enter
the following menu:

ENGINEER MENU	
BARO PRESS	760 mmHg
BALANCE GA	AIR
O2 CONCENT	20%
ANESTHETIC	00%
ZERO GAS	AIR
BTPS	DISABLE
SCREEN ROTATE	AUTO
LOAD DEFAULTS	
CALIBRATE	
EXIT	

Figure 10

In this menu to press button S to move the cursor to choose item,
to press button +/-  or button  to change data
highlighted by the cursor.

In this menu, press  button, to exit this menu and enter the
main display screen.

Some items of this menu can be directly adjusted, such as LOAD-

DEFAULT or EXIT: to press button to execute.

This menu including the following setups

BARO PRESS 760mmHg

BALANCE GAS: AIR, N2O, and HELIUM

O₂CONCENTRATION 20%-99%

ANAESTHETIC GAS 0-20%

ZERO GAS AIR, N₂

BTPS ENABLE, DISABLE

SCREEN ROTATE AUTO, MANUAL

LOAD DEFAULTS

CALIBRATE

Default values as follows:

BARO PRESS 760mmHg

BALANCE GAS AIR

O₂CONCENTRATION 20 %

ANAESTHETIC 0 %

GAS: ZERO GAS:

AIR BTPS: DISABLE

SCREEN ROTATE AUTO

Appendix3. Guidance and manufacturer's declaration -

Electromagnetic compatibility

Table 1 Guidance and manufacturer's declaration -

electromagnetic emission-for all EQUIPMENT AND SYSTEMS

This device is intended for use in the electromagnetic environment specified below. The customer or the user of the equipment or system should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment-guidance
RF emissions CISPR 11	Group 1	This device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	This device is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC61000-3-2	Class A	
Voltage fluctuations/flicker emissions IEC61000-3-3	Complies	

**Table 2 Guidance and manufacturer's declaration -
electromagnetic immunity for all EQUIPMENT AND SYSTEMS**

This device is intended for use in the electromagnetic environment specified below. The customer or the user of the equipment or system should assure that it is used in such an environment.			
Immunity test	IEC60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC61000-4-2	±6 kV contact ±8kV air	±6 kV contact ±8kV air	Floors should be wood, concrete or ceramic tile. if floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC61000-4-4	±2kV for power Supply lines ±1 kV for input/output lines	±2kV for power Supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1kV line(s) to line(s) ±2kV line(s) to earth	±1kV differential mode ±2kV common mode	Mains power quality should be that of a typical commercial or hospital environment.


User Manual of Mainstream Capnograph

<p>Voltage dips, short interruptions and voltage variations on power supply input lines IEC61000-4-11</p>	<p><5%UT (>95% dip in UT) for 0,5 cycle 40% UT (60% dip in UT) for 5 cycles 70% UT (30% dip in UT) for 25 cycles <5% UT (>95% dip in UT) for 5 s</p>	<p><5%UT (>95% dip in UT) for 0,5 cycle 40% UT (60% dip in UT) for 5 cycles 70% UT (30% dip in UT) for 25 cycles <5% UT (>95% dip in UT) for 5 s</p>	<p>Mains power quality should be that of a typical commercial or hospital environment. If the user of the equipment or system requires continued operation during power mains interruptions, it is recommended that the equipment or system be powered from an uninterruptible power supply or a battery.</p>
<p>Power frequency (50Hz/60Hz) magnetic field IEC61000-4-8</p>	<p>3A/m</p>	<p>3A/m</p>	<p>Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.</p>
<p>NOTE: UT is the a.c. mains voltage prior to application of the test level.</p>			

**Table 3 Guidance and manufacturer's declaration –
electromagnetic immunity-for EQUIPMENT and SYSTEM that
are not LIFE-SUPPORTING**

This device is intended for use in the electromagnetic environment specified below. The customer or the user of this device should assure that it is used in such an electromagnetic environment.			
IMMUNITY test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3V 3 V/m	Portable and mobile RF communications equipment should be used no closer to any part of this device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d=1.2 \sqrt{P}$ $d=1.280\text{MHz}-800\text{MHz}$ $d=2.3800\text{MHz}-2.5\text{GHz}$ Where P is the maximum output power rating of the transmitter in watts (W) according to the manufacturer and d is the recommended
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz		

User Manual of Mainstream Capnograph

			<p>separation distance in meters (m). b Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, a should be less than the compliance level in each frequency range .b Interference may occur in the vicinity of equipment marked with the following symbol.</p> 
--	--	--	--

NOTE 1: At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

a: Field strengths from fixed transmitters, such as base stations for radio (cellular / cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which this device is used exceeds the applicable RF compliance level above, this device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating this device.

b: Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3V/m.

User Manual of Mainstream Capnograph

Table 4 Recommended separation distances between portable and mobile RF communications equipment and the equipment or system-for EQUIPMENT and SYSTEM that are not LIFE-SUPPORTING

This device is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the equipment or system can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the equipment or system as recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter (W)	Separation distance according to frequency of transmitter (m)		
	150kHz to 80MHz d=1.2	80MHz to 800MHz d=1.2	800MHz to 2,5GHz d=2.3
0,01	0.12	0.12	0.23
0,1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be determined using the equation applicable to the frequency of the transmitter, where p is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer. NOTE 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies. NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			