



DISPOSABLE CONTAINERS FOR SUCTION APPLICATIONS FLO VAC

CONTAINER WITH MECHANICAL VALVE

flow-meterTM
ENGINEERING REVOLUTION IN MEDICAL TECHNOLOGY

FLOVAC® DISPOSABLE CONTAINERS SYSTEM FOR THE COLLECTION OF SUCTIONED FLUIDS

The **FLOVAC** disposable containers system is designed and manufactured for “high flow and high vacuum” applications in a medical suction field to collect the organic fluids. This system is the best expression of safety, practicality and simplicity of use, both for the operators and for hospital plants and environment, thanks to the use of absolutely reliable manufacturing materials. The hermetic lid sealing makes the disposal procedure particularly hygienic, simple and safe for the patient and for the staff charged to remove and handle the device. The replacement operations are very simple, reducing to the minimum the plant stops in each application. Moreover, flow-meter T designed and developed a complete range of accessories aimed at covering the most of hospital applications.

FLOVAC® DISPOSABLE CONTAINERS TWO VERSIONS:



LINER

A disposable soft liner bag in 3 sizes hermetically welded to a rigid lid. This bag has to be placed in the related **FLOVAC**® system PC reusable and autoclavable support rigid container.



CANISTER

A complete disposable system. A single-use rigid canister in 3 sizes and a lid coupled with spring clips to prevent any accidental opening and to give hermetical sealing.

PRACTICALITY
SAFETY
SIMPLICITY



LINER AND CANISTER VERSIONS ARE:

Available in three sizes: 1.0 L, 2.0 L and 3.0 L.

Supplied (option) in package with 1.8 m hose or with 1.8 m hose and vacuum breaker.

Equipped with ports allowing the connection to the suction line (female), to the patient (male connection), plus the possibility to increase the collection capacity by using two or more containers connected in cascade.

Equipped with a mechanical overflow valve and with an antibacterial filter to protect the suction equipment or the patient from contamination.

TANDEM PORT

HOW TO INCREASE THE CAPACITY OF SUCTIONED FLUIDS COLLECTION BY CONNECTING IN CASCADE MORE CONTAINERS

According to the fluid volume expected to be suctioned, the system gives 3 options of sizes. In case the volume is exceeding the maximum size available, it is possible to increase the capacity through the **TANDEM** port. This allows the cascade connection of two or more containers, increasing dramatically the system collection capacity.



TECHNICAL CHARACTERISTICS

LINER

Soft bag material: LDPE
(Low Density Polyethylene).

Lid: HDPE
(High Density Polyethylene).

Individually packed in blisters.

CANISTER

Jar material: High-Clarity PP
(High Clarity Polypropylene).

Lid: HDPE
(High Density Polyethylene).

Connection between jar and lid through
pressure seal with permanent fastening
spring clips.

Jar storage using concentric cone
system with 4 lower blocking ribs.




FLOVAC® MECHANICAL VALVE

Lid material	HDPE (High Density Polyethylene)
VACUUM port	conic female connection with ON-OFF function
PATIENT port	male connection Ø 14.0 ÷ 15.5 mm (Ø 8.0 ÷ 9.2 mm with elbow connector)
TANDEM port	male Ø 8.0 ÷ 9.2 mm connection
Maximum suction value	-750 mbar (-570 mm Hg)
Maximum flow value	42 L/min. under recommended conditions
Jar external scale graduation	500 ml intervals
Patient hose size	inner Ø ≥ 6 mm (recommended Ø 7.5x11.2 mm - L=2.5 m max)
Vacuum hose size	inner Ø ≥ 6 mm - L=1.8 m max
Overflow valve	mechanical float type
Filter	antibacterial



THE FLOVAC® LID

The lids are obviously different between the **LINER** version, having the collection bag welded and integrated, and the **CANISTER** version, where the lid is a cover able to get complete sealing when firmly placed and connected onto the jar. In both **FLOVAC®** versions all connections and handling devices are concentrated on the lid. **PATIENT** and **VACUUM** ports (one male and the other female with ON-OFF function, to avoid any misconnection), the **TANDEM** port, the handle to help the bag removal after use (**LINER** version) and for easy transport, two plugs, connected to the lid through integrated plastic wirings, to close and seal the **PATIENT** port and the **TANDEM** port after use. In case of suction with one jar only, this **TANDEM** port must be plugged before use. The male **PATIENT** port fits a removable 90° elbow with connection diameter 8.0÷9.2 mm for normal suction operations. In case of suction with expected collected fluids containing bone fragments it is enough to remove the elbow getting access to the direct vertical connecting port having diameter 14.0÷15.5 mm. The lower part of the lid fits the overflow mechanical valve with integrated

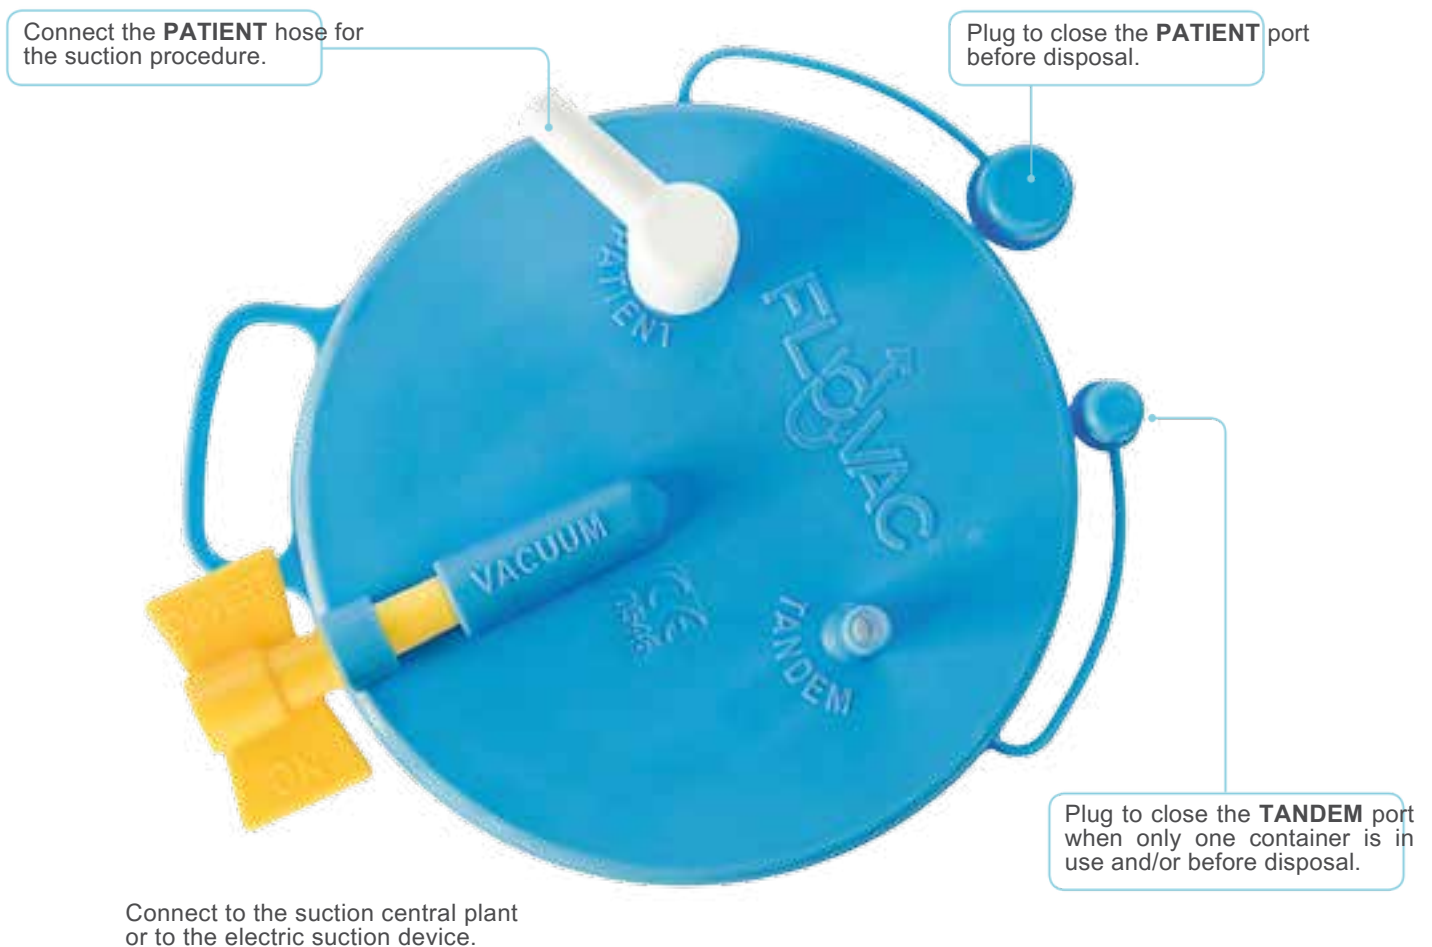

THE FLOVAC® JAR

The jars too are obviously different between the **LINER** version, where the **PC** reusable jar has the function to support the disposable bag, and the **CANISTER** version, where the jar, when fastened with the lid, becomes a complete sealed container to be disposed after the use. In both versions a graduated scale printed outside the jar allows an easy monitoring of the volume of the suctioned fluid. The jars, both in **LINER** and **CANISTER** versions, have a conical shape to get small size packaging, to save transport costs and space during the storage. To avoid jars getting stuck or unexpected inner scraping, four ribs inside the bottom area stop properly the jar position when one inside the other.

LINER



CANISTER



FLOVAC® MECHANICAL VALVE

IN DETAIL



1 CANISTER lid fixing - The **FLOVAC®** container lid in the **CANISTER** version fits 5 spring clips to grant a permanent and safe fastening to the rigid jar to prevent any leakage and the accidental opening. Never try to reopen the container when lid placed and clips fastened. An eventual second closing cannot guarantee sealing and accidental opening.

2 PATIENT port - The **PATIENT** port allows the suction of fluids

3 containing bones fragments, once the elbow connector is removed.

VACUUM connector - The vacuum source coming from the

4 plant or from an

ephoelser, hct i cfratorolrus e cgastayh, uspil oemnes ,aiPmshap fteCdnierf althines VnAbObUcdionMnenn

safe **FLOVAC®** container connection and disconnection.

5 Suction kit - The full **FLOVAC®** collection containers range is also available in

odpistpioons awbilteh vaa c1u.u8m m disposable suction hose, or 1.8 m hose plus breaker. **Support ring** - The **FLOVAC®** support ring is the same

6 for the 2 versions, **LINER**

and **CANISTER**, the 3 sizes 1, 2, 3 liters and the different fitment: wall, rail, trolley.

A the psruinctgio cnl itpu binet egrated in the external diameter of the ring allows

7 to be easily fixed in to avoid obstructions. **VACUUM port** - This connection to the vacuum source is conical to guarantee




anpade "rffeemcta cleo"n tact sealing, to get simple connection and removing


8 to avoid any misconnection with the **PATIENT** "male" port. This

possibility exists

hine aclaths es taofff snteawrts **FLOVAC®** system installations or when new practicing with the system. The different ports connection avoids this possibility.

8 Mcloosreeo tvheer ptohret vacuum port is equipped with an ON-OFF switch to after use and before disposal to grant a perfect sealing. **TANDEM**

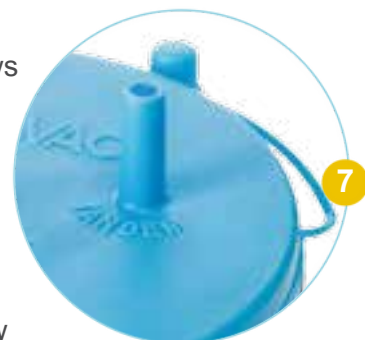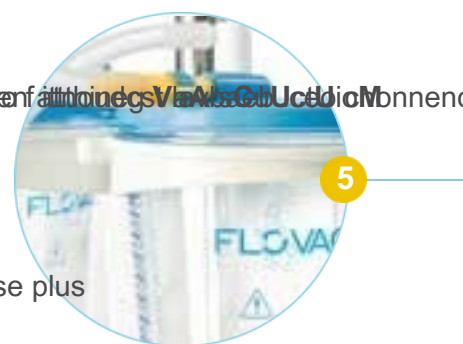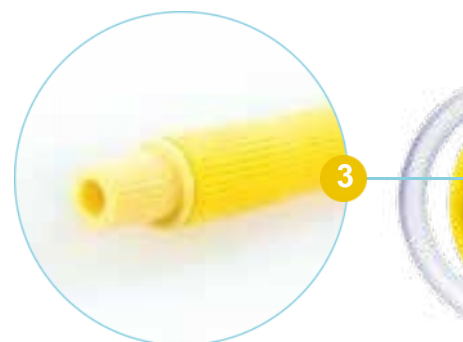

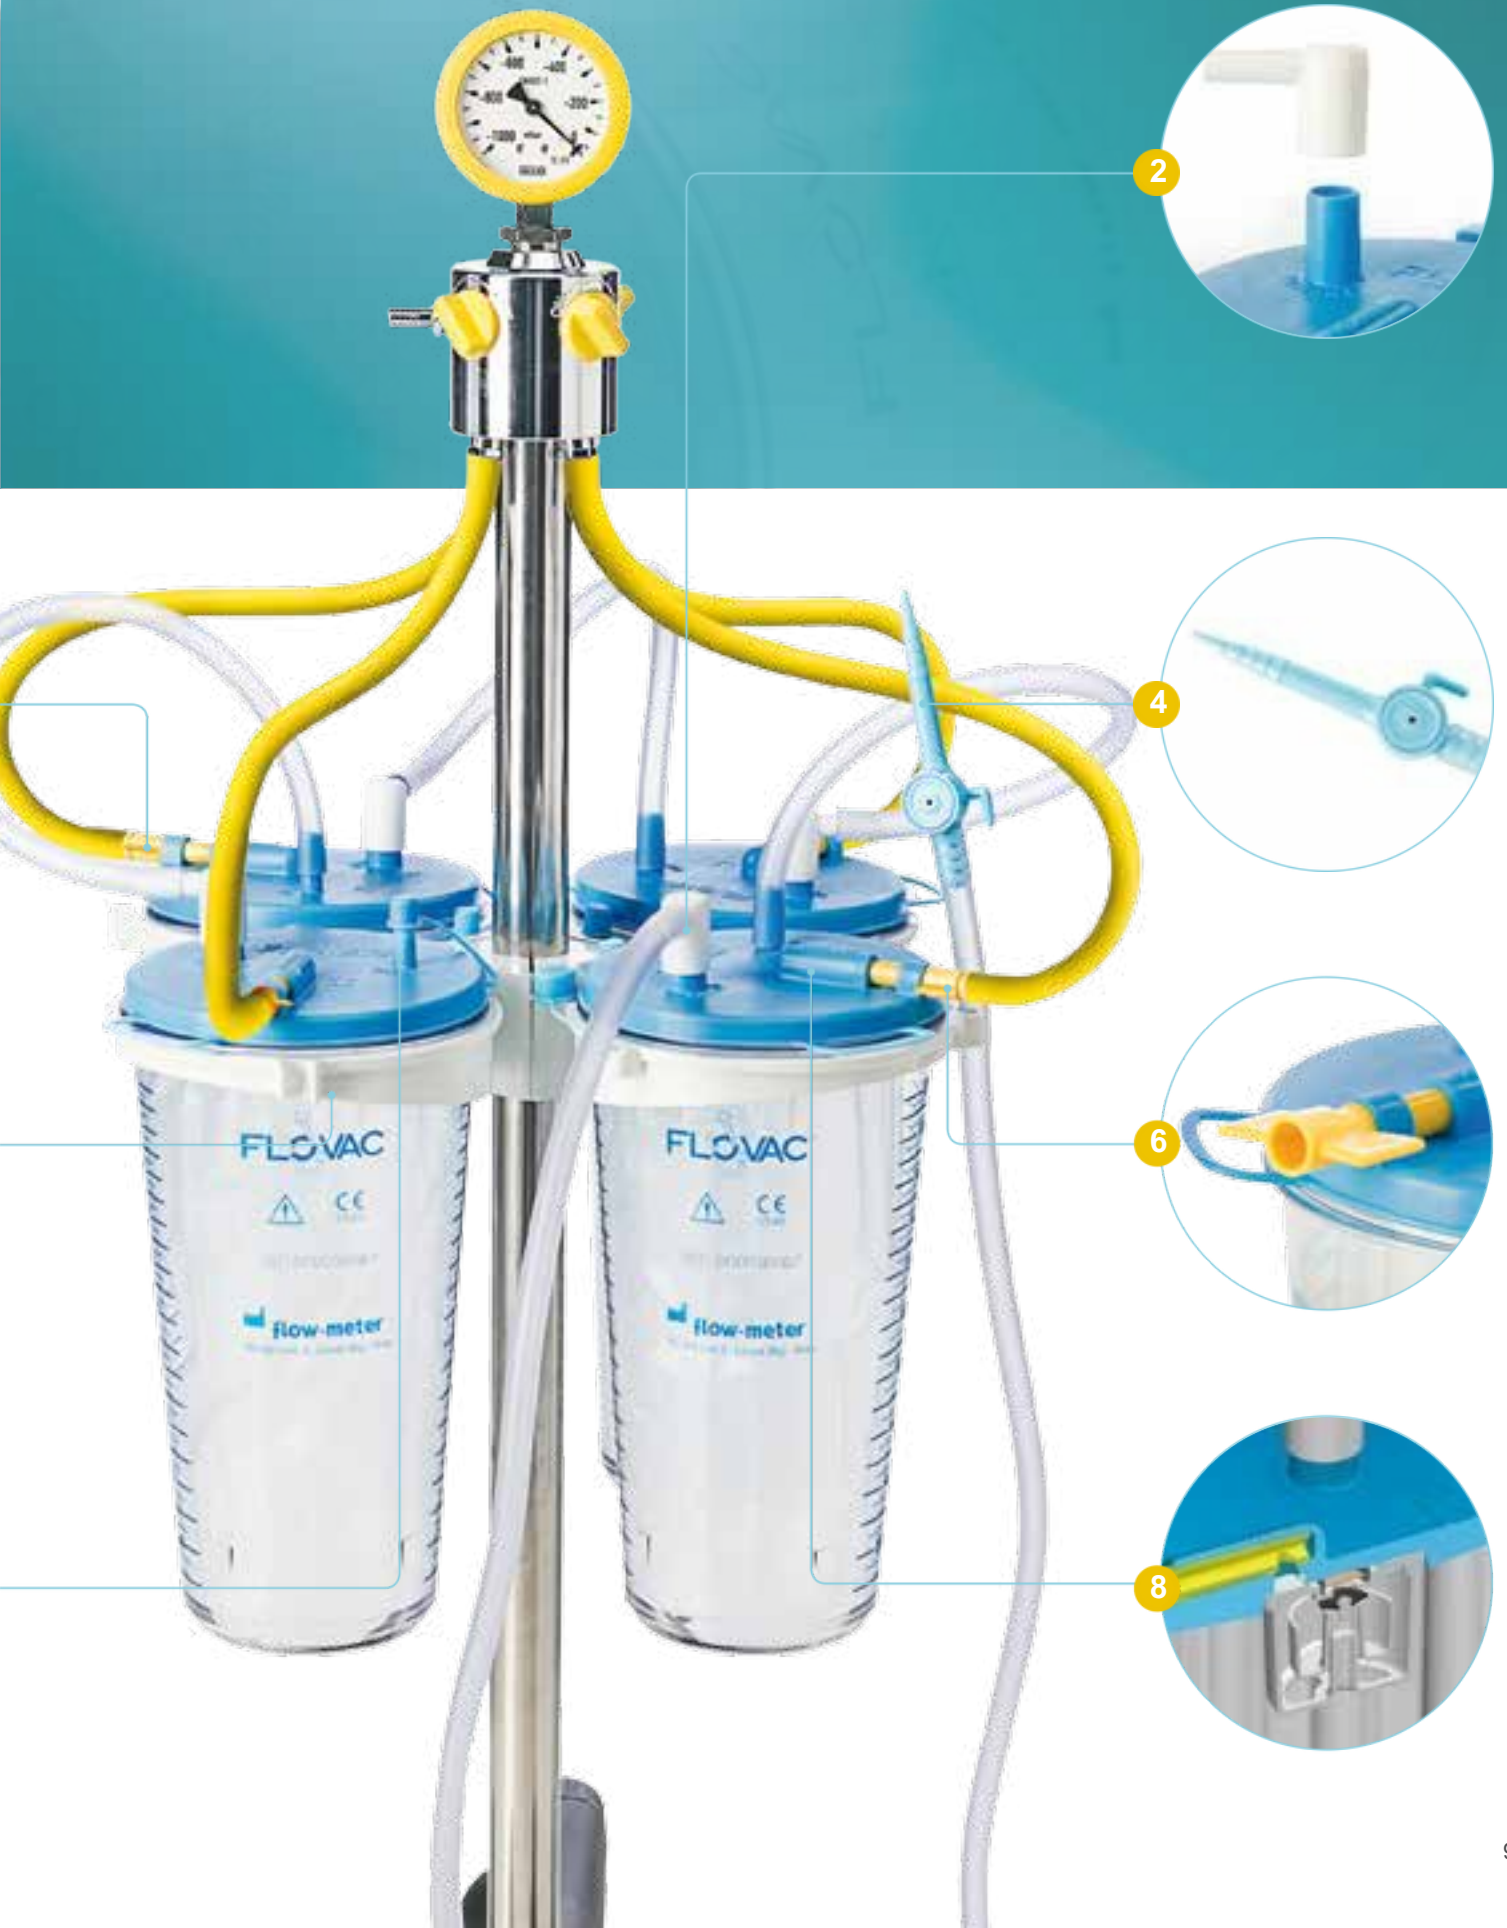

GELLING KIT

HOW DOES IT WORKS?

The **gelling kit** gives further safety to an highly efficient system. It is a special absorbing powder transforming liquids in a semi-solid mass. This grants handling with higher safety for operators charged to clean, handle and transport potentially infected materials. This process allows to absorb and incorporate all liquids suctioned in the **FLOVAC®** containers and to prevent dangerous contamination risks for the health staff in case of biological fluids accidental leakage.



GELLING POWDER

The correct necessary quantity of gelling powder is supplied in small water-soluble pouches, already inserted into the container bag in **LINER** version, or supplied in 50 pieces boxes for use in **CANISTER** version. In this case one single gelling bag needs to be placed into the container before fastening the lid.

APPLICATIONS IN TANDEM

When suction is made with collection systems using prefilled gelling kit, **LINER** or **CANISTER** versions, it is not recommended to use the containers connected in **TANDEM**. For applications in **TANDEM**, the gelling powder is available in 500 g. bottles with funnel/doser so that to be poured into the **FLOVAC®** containers by the operators after the use and before disposal.



Gellified suctioned liquid.

Soft bag made in LDPE (Low Density Polyethylene).

Jar made in High Clarity Polypropylene.



ACCESSORIES FLOVAC®

DISPOSABLE CONTAINERS



Reusable support jars (**LINER** version) 1.02 L, 2.0 L, 3.0 L in polycarbonate, autoclavable



Support ring for **FLOVAC®** container with 25x5 mm hook (standard) with 30x5 mm hook with 41x4 mm hook with 45x5 mm hook.



ON-OFF tap with or without control vacuum gauge for fitting **FLOVAC®** container support ring.



Bracket for 30x10 mm rail in technopolymer with 25x5 mm slide.



Reusable polycarbonate connector to supply the **VACUUM** port.
25 pieces/box



Hoses Ø 7.5x11.2 mm - L=0.38 m with connector to supply the **VACUUM** port.
50 pieces/box



Hoses Ø 7.5x11.2 mm - L=0.38 m for **TAND** connection.
50 pieces/box



TANDEM connection system.
100 pieces/box



"T" connector for wall **TANDEM** applications.
100 pieces/box



Specimen container.
10 pieces/box



Gelling powder in 500 g. bottles with funnel/
10 bottles/box



Disposable **VACUUM** breaker.
50 pieces/box



Hose Ø 7.5x11.2 mm - L=1.8 m with disposable
VACUUM breaker.
100 pieces/box



Special gelling powder bag for all sizes
of **CANISTER FLOVAC®**.
50 pieces/box

ACCESSORIES FLOVAC®

DISPOSABLE CONTAINERS



4-places trolley for **FLOVAC®** container with 4 support rings, ON-OFF taps and vacuum regulator.

4-places trolley for **FLOVAC®** container with 4 support rings, and handle.

flow-meter™
ENGINEERING REVOLUTION IN MEDICAL TECHNOLOGY

Via del Lino, 6 24040
Levate - Bergamo ITALY

info@flowmeter.it

www.flowmeter.it
flovac.flowmeter.it

Ph. +39 035 594047

Fax +39 035 594821